
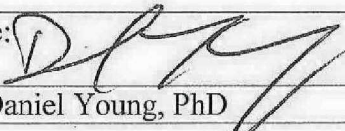


<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	CLIA Laboratory	Effective Date: 11/26/2013
Proficiency testing for Theranos Lab-Developed Tests: Edison 3.5		

**Author(s):**

Signature: 	Date: 12-2-13
Name: Li Ding-Chiang	Title: Laboratory General Supervisor

**Reviewer(s)**

Signature: 	Date: 12/2/2013
Name: Daniel Young, PhD	Title: Vice President

**Approver(s):**

Signature: 	Date: 12/2/2013
Name: Adam Rosendorff, M.D	Title: Laboratory Director

Theranos Internal Only

COPY

**CONTROLLED DOCUMENT**

Theranos Confidential	Page 1 of 8
-----------------------	-------------

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

CL SOP-19001 Rev. A, Released Date 10/23/2013

<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	CLIA Laboratory	Effective Date: 11/26/2013
<b>Proficiency testing for Theranos Lab-Developed Tests: Edison 3.5</b>		

**TABLE OF CONTENTS**

1 **PURPOSE**.....3  
 2 **SCOPE** .....3  
 3 **RESPONSIBILITIES** .....3-4  
 4 **PROCEDURE** .....5  
 5 **ACCEPTANCE CRITERIA**.....5  
 6 **RECORDS**.....6  
 7 **REFERENCES**.....6  
 8 **REVISION HISTORY**.....5

Theranos Internal Only

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

CL SOP-19001 Rev. A, Released Date 10/23/2013

<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	CLIA Laboratory	Effective Date: 11/26/2013
<b>Proficiency testing for Theranos Lab-Developed Tests: Edison 3.5</b>		

## 1 Purpose

- 1.1 The purpose of this proposal is to devise an alternative assessment protocol (AAP) for laboratory-developed tests on the EDISON 3.5 immunoassay instrument.
- 1.2 Guideline: For non-CMS-regulated tests or those which lack FDA clearance, commercial or external PT programs may not be available for certain analytes. In such instances, an AAP may help validate the quality of ongoing test system performance.

## 2 Scope

- 2.1 The alternative assessment protocol (AAP) applies to all laboratory developed tests on the EDISON 3.5 instrument, and will be conducted immediately following the receipt of proficiency testing results from the American Proficiency Institute (API). The API conducts proficiency testing of all 4 Immunoassays offered at time of SOP drafting (tPSA, 25-OH Vit D, TSH, ft4) three times a year. The AAP should be conducted minimally every 6 months.

## 3 Responsibilities

- 3.1 It is the responsibility of the technical supervisor (TS), to ensure that the alternative assessment procedure (AAP) is conducted at least twice times a year for all 4 analytes.
- 3.2 Laboratory Testing Personnel are responsible for the following:
- 3.2.1 Receiving and processing the proficiency testing samples from in-house patient collections.
  - 3.2.2 Reporting the results to the TS or designee for evaluation
  - 3.2.3 Completing applicable fields on CL FRM-00006-F1 *Proficiency Testing Evaluation*
- 3.3 The Laboratory Technical Supervisor is responsible for the following:
- 3.3.1 Making sure that proficiency testing samples are identified and prepared for the Laboratory
  - 3.3.2 Ensuring that over a 12 month PT cycle, samples representing the entire range of each

Theranos Confidential

Page 3 of 8

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

CL SOP-19001 Rev. A, Released Date 10/23/2013

<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	CLIA Laboratory	Effective Date: 11/26/2013
<b>Proficiency testing for Theraanos Lab-Developed Tests: Edison 3.5</b>		

assay are selected and submitted for testing

3.3.3 Evaluating proficiency testing sample results

3.3.4 Completing applicable fields on CL FRM-00006-F1 *Proficiency Testing Evaluation*

3.4 The Laboratory Director is responsible for the following:

3.4.1 Reviewing and approving each PT testing event documentation.

Theraanos Internal Only

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	CLIA Laboratory	Effective Date: 11/26/2013
<b>Proficiency testing for Theranos Lab-Developed Tests: Edison 3.5</b>		

#### 4 Procedure

- 4.1 Obtain 5 venous clinical samples from an in-house collection.
- 4.2 At least 10mL of K2-EDTA anticoagulated blood should be collected.
- 4.3 Split the samples into 2 aliquots
- 4.4 Run the predicate Siemens Immulite 2000 and Theranos LDT methods in parallel, using n=5 for each assay, for each patient sample.
- 4.5 Calculate the mean, SD and % CV for each analyte on each method.
- 4.6 Calculate the average bias of the Theranos LDT test as follows: Average bias = mean (Theranos)-mean (Immulite)/mean (Immulite)
- 4.7 In the event that analyte samples, as determined by the predicate method, do not span the a clinically relevant medical decision level (CL-DOC-95010 (Appendix I), clinical samples should be supplemented ("spiked") with exogenous analyte to bring it into range.
- 4.8 Sufficient clinical sample material should be collected to perform additional level testing n=5 for each assay.

#### 5 Acceptance criteria

- 5.1 The sum of the %CV and the average bias should not exceed the total allowable error stated in CL-DOC-95010 (Appendix I).
- 5.2 If an analyte fails >20% (>1 out of 5) of the patient clinical samples, then the proficiency will be deemed to have failed the proficiency event.
- 5.3 If an analyte fails a proficiency event, corrective actions will be implemented, according to QOP-00006
- 5.4 If an analyte fails two consecutive proficiency events, testing will be discontinued for that analyte, until such time as the assay is corrected, and passes AAP PT re-testing.
  - 5.4.1 The latter event will be documented and signed off by the laboratory director

Theranos Confidential	Page 5 of 8
-----------------------	-------------

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

CL SOP-19001 Rev. A, Released Date 10/23/2013

<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	<b>CLIA Laboratory</b>	Effective Date: 11/26/2013
<b>Proficiency testing for Theranos Lab-Developed Tests: Edison 3.5</b>		


5.4.2 Resumption of testing will only occur upon documentation and approval by the laboratory director.

**6 RECORDS**

6.1 All PT records will be retained for a minimum of 3 years

**7 REFERENCES**

- 7.1 42 CFR Part 493 Subpart H, Participation in Proficiency Testing for Laboratories Performing Tests of Moderate Complexity (Including the Subcategory), High Complexity, or Any Combination of These Tests
- 7.2 42 CFR Part 493.1236, Standard: Evaluation of proficiency testing performance
- 7.3 42 CFR Part 493.1445, Standard: Laboratory Director Responsibilities
- 7.4 CLSI Guideline GP27
- 7.5 CLSI Guideline GP 29

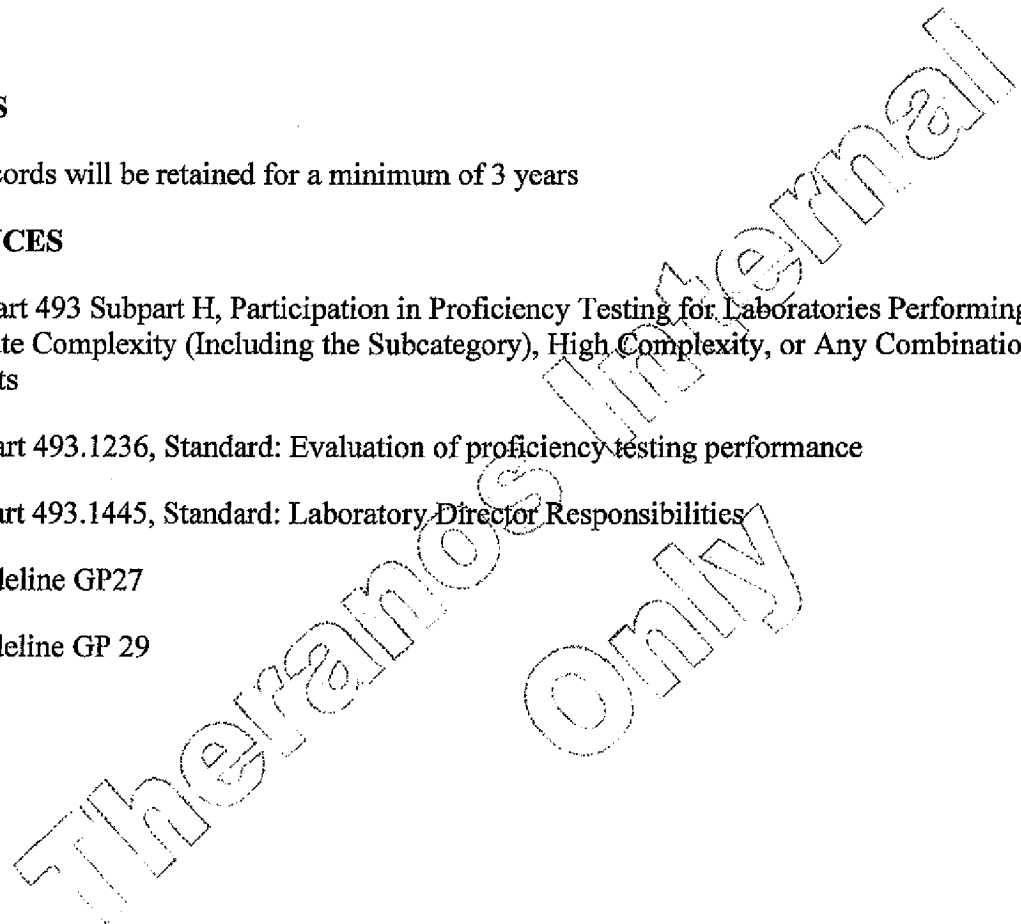

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

CL SOP-19001 Rev. A, Released Date 10/23/2013

<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	CLIA Laboratory	Effective Date: 11/26/2013
<b>Proficiency testing for Theranos Lab-Developed Tests: Edison 3.5</b>		

**8 REVISION HISTORY**

<b>REVISION HISTORY</b>			
<b>Revision Level</b>	<b>Effective Date</b>	<b>Initiator</b>	<b>ECO Number</b>
A	11/26/2013	A. Rosendorff	ECO-000126
<b>Section Number</b>	<b>Description and Justification of Changes</b>		

Theranos Internal Only

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

CL SOP-19001 Rev. A, Released Date 10/23/2013

<b>theranos</b>	<b>Standard Operating Procedure</b>	Document Number: CL SOP-00020
	CLIA Laboratory	Effective Date: 11/26/2013
<b>Proficiency testing for Theranos Lab-Developed Tests: Edison 3.5</b>		

Theranos Internal  
Only

Any retransmissions, reproductions, dissemination or other use of these materials by persons or entities other than the intended recipient is prohibited. This document supersedes all earlier or previous documents unless approved in writing.

CL SOP-19001 Rev. A, Released Date 10/23/2013